



**NOTES:**

1. FLOW PATH VALVE ENERGIZED: — — —  
FLOW PATH VALVE DE-ENERGIZED: ———
2. R1 (.004" I.D.) MATCHES RESTRICTION OF COL. 3.
3. DELETED PER ECO-XX-5001213.
4. V1/5 TO V2/5: USE 0.020 ID TUBING.
5. OPTIONAL 4 OR 8 STREAMS; STREAM 1 IS THE CALIBRATION INPUT.
6. INSTALL 3" OF .004 ID 1/16 TUBING FOR FLOW RESTRICTION.
7. INSTALL 3" OF .004 ID 1/16 TUBING FOR FLOW RESTRICTION AT VALVE. USE CAPILLARY COUPLER AND .043 ID TUBING TO EXTEND TO DETECTOR.

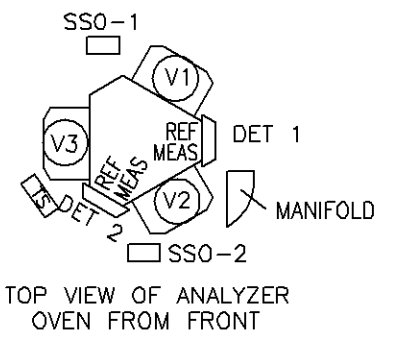

SSO-1 & -2 WIRING

SI METRIC							
THIRD ANGLE PROJECTION							
MATERIAL		N/A					
FINISH		N/A					
PROJ. FILE NO. G-00001	FILENAME: CE25002-001A1.DWG, DATE: 05/05/09, TIME: 4:30 P.M.	A	05/05/09	CC	RELEASED	EM	DLT
REV	DATE	DRN	DESCRIPTION	CHKD	APPD		

THIS DRAWING IN DESIGN AND DETAIL IS OUR PROPERTY AND MUST NOT BE USED EXCEPT IN CONNECTION WITH OUR WORK. IT SHALL NOT BE REPRODUCED AND SHALL BE RETURNED TO US ON DEMAND. ALL RIGHTS ARE RESERVED.

GEOMETRIC TOLERANCES & DIMENSIONS PER ANSI Y14.5 LATEST REVISION

UNLESS OTHERWISE NOTED ALL DIMENSIONS IN INCHES  
 X.XX ±.015  
 X.XXX ±.005  
 ANGULAR ±0° 30'  
 FINISH 200 RA MAX

BREAK ALL SHARP CORNERS TO .003-.015 RADIUS AND REMOVE ALL BURRS

**EMERSON**  
Process Management

TITLE  
 FLOW CONFIGURATION  
 DET. 1: B/F TO MEAS. D/C  
 DET. 2: B/F TO MEAS.  
 MODEL 700  
 CAL 1 = STREAM 1

DRN	CC	DATE	05/05/09	DWG NO.	CE-25002-001	REV	A
CHKD	EM	DATE	05/05/09	SCALE	NTS	P/N	SEE ORDER
APPD	DLT	DATE	05/05/09	SCALE	NTS	P/N	SEE ORDER

SHT 1 OF 1