


- ③ WELD PROTECTION TO BE REMOVED AFTER WELD WORK.
- ② MARK GROOVE MUST BE DIRECTED OUT FROM THE TANK.
- ① REC. WELDING PIN Ok6770, Ok6771, Ok6775, AWS: A/SSA 5.4 E309L, AWS: A/SSA 5.4 E309MoL. WELD DIMENSION IS ONLY RECOMMENDED. FOR PRESSURED APPLICATIONS SEE NATIONAL STANDARDS AND PRACTISE.

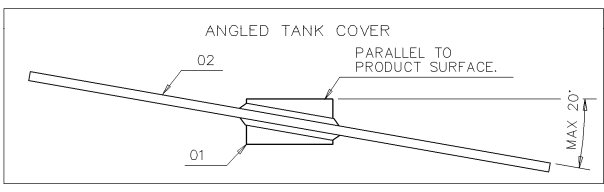

03	WELD PIN	-	SEE NOTE 1.	CUSTOMER
02	TANK FLANGE/COVER	1		CUSTOMER
01	FLANGE BALL T38-W	1	AISI 316L	RTR
POS	ITEM DESCRIPTION	QTY	REMARK	SUPPLIER
ISSUED BY	WEEK	PRODUCT CODE	FILE	INSTALLATION DRAWING TITLE
GU-HF	0307	REX	ACAD	MECHANICAL INSTALLATION DWG
APPROVED BY	WEEK	ORIGINAL DWG NO.	SCALE	FLANGE BALL T38-W, WELDING
GST-TK	0307	9240003-944	-	
ROSEMOUNT		1 ST ANGLE	DOC TYPE	DWG NO.
Tank Gauging			2	9240003-944
THE COPYRIGHT/OWNERSHIP OF THIS DOCUMENT IS AND WILL REMAIN OURS. THE DOCUMENT MUST NOT BE USED WITHOUT OUR AUTHORIZATION OR BROUGHT TO THE KNOWLEDGE OF A THIRD PARTY. COPIRIGHT INFRINGEMENT WILL BE PROSECUTED. ROSEMOUNT TANK RADAR AB, SWEDEN.				ISSUE
				3
				SHEET
				1/1